

AlphaLISA® Research Reagents

Caution: For Laboratory Use. A research chemical for research purposes only

Protein A Alpha Donor Beads

Product No.: AS102D (1 mg)

AS102M (5 mg) AS102R (25 mg)

Lot No.: P1

Product Formats

Catalog #	Size	Volume	Assay Points*
AS102D	1 mg	200 µL	2 000
AS102M	5 mg	1 mL	10 000
AS102R	25 mg	5 mL	50 000

^{*} The number of assay points is based on an assay volume of 25 μL using a final bead concentration of 20 μg/mL in 384-well format.

Manufacturing Date: March 04, 2011

Product Information

Description: Protein A Alpha Donor beads at 5 mg/mL in PBS pH 7.2 with 0.05% Proclin-300 as a

preservative. The protein used is a native protein.

Application: This product is intended for use in homogeneous AlphaLISA assays to capture Fc region of IgG

of several species (human IgG, human IgM, mouse IgG and rabbit IgG). AlphaLISA Acceptor

beads must be ordered separately.

Storage: Store in the dark at 4°C.

Stability: This product is stable for at least 12 months from the manufacturing date when stored in its

original packaging under recommended storage conditions. Diluted beads are light-sensitive.

Therefore, beads must be used immediately after dilution.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

Quality Control

Lot-to-lot consistency is confirmed by a Quality Control AlphaLISA titration assay read on an EnVision[®] HTS Alpha instrument (see protocol below). We certify that the results meet our quality release criteria. *Note: maximum counts will vary depending on assay conditions as well as between lots. This variation has no impact on assay quality.*

Maximum signal: 243 925 counts Minimum signal: 305 counts EC_{50} : 0.056 nM



Titration Assay (Quality Control Protocol)

This protocol provides a means to verify product performance. It is used as our Quality Control release test. The following reagents and materials are used:

Item	Suggested Source	Catalog #
Streptavidin AlphaLISA Acceptor beads	PerkinElmer	AL125C (250 μg) AL125M (5 mg) AL125R (25 mg)
Biotinylated Rabbit IgG	Jackson ImmunoResearch	011-060-003
AlphaLISA Universal Assay Buffer, 5X	PerkinElmer	AL001C (10 mL) AL001F (100 mL)
White OptiPlate™-384	PerkinElmer	6007290
TopSeal™-A Adhesive Sealing Film	PerkinElmer	6005185
EnSpire [®] or EnVision Multilabel Alpha Reader	PerkinElmer	-

Recommendations

- The volume indicated on each tube is guaranteed for single pipetting. Multiple pipetting of the reagents may reduce the theoretical amount left in the tube. To minimize loss when pipetting beads, it is preferable not to prewet the tip.
- Alpha Donor beads are light-sensitive. All steps using the Alpha Donor beads should be performed under subdued laboratory lighting (< 100 lux). Green filters (Roscolux filters #389 from Rosco, or the equivalent) can be applied to light fixtures. All the other assay reagents can be used under normal light conditions.
- Sodium azide should not be added to stock reagents. High concentrations of sodium azide (> 0.001 % final in the assay) might decrease the AlphaLISA signal.
- Centrifuge the tubes briefly before use to improve recovery of content (2,000 x g, 10-15 sec). Resuspend all reagents by vortexing before use.
- Use Milli-Q[®] grade water (18 MΩ•cm) to dilute the 5X AlphaLISA Universal Assay Buffer.
- When diluting the probe, change tips after each dilution. When loading reagents in the assay microplate, change tips after each reagent addition and between each set of reagents.
- When reagents are added in the microplate, make sure the liquids are at the bottom of the well.
- 1X AlphaLISA Universal Assay Buffer contains PBS, pH 7.5, 0.1% BSA, 0.01% Proclin-300. This buffer is used in the titration assay described below (Quality Control Protocol). Optimization of the assay buffer might be necessary in other assay types.
- Small volumes may be prone to evaporation. It is recommended to cover microplates with TopSeal-A Adhesive Sealing Film to reduce evaporation during incubation. Microplates are read with the TopSeal-A Film on the plate.
- Total signal varies with temperature and incubation time. For consistent results, identical incubation times and temperature should be used for all plates.



The AlphaLISA signal is detected with an Alpha-enabled EnSpire or EnVision Multilabel Reader using the AlphaScreen standard settings (e.g. Total Measurement Time: 550 ms, Laser 680 nm, Excitation Time: 180 ms, Mirror: D640as, Emission Filter: M570w, Center Wavelength 570 nm, Bandwidth 100 nm, Transmittance 75%).

Quality Control Protocol

This titration protocol is designed for 12 dilutions of the probe with triplicate determinations. Final concentration of AlphaLISA Acceptor and Alpha Donor beads in the 25 uL final assay volume is 20 ug/mL. Volume of diluted reagents should be adjusted according to total number of assay points, plate format or assay volume.

- Preparation of 1X AlphaLISA Universal Assay Buffer: Add 1 mL of 5X AlphaLISA Universal Assay Buffer to 4 mL H₂O.
- Preparation of 1.7X probe (Biotinylated Rabbit IgG) dilutions: 2) Dilute probe to a 50 nM stock solution. Prepare dilution series in 1X AlphaLISA Universal Assay Buffer as follows, changing tip for each dilution:


	Volume of Probe	Volume of 1X Buffer (μL)	[Biotinylated Rabbit IgG] (M)		
Tube			in 15 μL (1.7X)	in 25 μL Final Assay Volume	
Α	5 μL of 50 nM	141	1.7E-09	1.0E-09	
В	60 μL of tube A	140	5.1E-10	3.0E-10	
С	60 μL of tube B	120	1.7E-10	1.0E-10	
D	60 μL of tube C	140	5.1E-11	3.0E-11	
Е	60 μL of tube D	120	1.7E-11	1.0E-11	
F	60 μL of tube E	140	5.1E-12	3.0E-12	
G	60 μL of tube F	120	1.7E-12	1.0E-12	
Н	60 μL of tube G	140	5.1E-13	3.0E-13	
I	60 μL of tube H	120	1.7E-13	1.0E-13	
J	60 μL of tube I	140	5.1E-14	3.0E-14	
K	60 μL of tube J	120	1.7E-14	1.0E-14	
L	0	140	0	0	

Preparation of 5X Alpha Donor beads (100 µg/mL): Diluted beads are light-sensitive. Therefore, beads must be used immediately after dilution. Add 5 µL of 5 mg/mL Alpha Donor beads to 245 µL of 1X AlphaLISA Universal Assay Buffer.


4) Preparation of 5X AlphaLISA Acceptor beads (100 μg/mL): Add 5 µL of 5 mg/mL AlphaLISA Acceptor beads to 245 µL of 1X AlphaLISA Universal Assay Buffer.



5) <u>In a white opaque OptiPlate-384 microplate:</u>

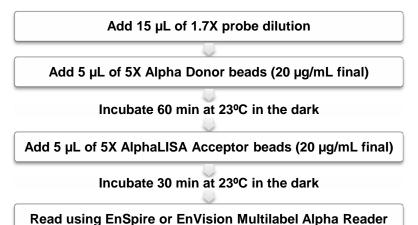

Typical Product Data

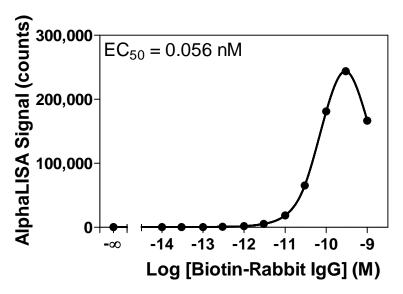

Titration assay using the Quality Control protocol. Signal was detected with an EnVision Alpha instrument 2102.

Please visit our website for additional information on the AlphaLISA technology at www.perkinelmer.com/AlphaTech.

This product is not for resale or distribution except by authorized distributors.

LIMITED WARRANTY: PerkinElmer BioSignal Inc. warrants that, at the time of shipment, the products sold by it are free from defects in material and workmanship and conform to specifications which accompany the product. PerkinElmer BioSignal Inc. makes no other warranty, express or implied with respect to the products, including any warranty of merchantability or fitness for any particular purpose. Notification of any breach of warranty must be made within 60 days of receipt unless otherwise provided in writing by PerkinElmer BioSignal Inc. No claim shall be honored if the customer fails to notify PerkinElmer BioSignal Inc. within the period specified. The sole and exclusive remedy of the customer for any liability of PerkinElmer BioSignal Inc. of any kind including liability based upon warranty (express or implied whether contained herein or elsewhere), strict liability contract or otherwise is limited to the replacement of the goods or the refunds of the invoice price of goods. PerkinElmer BioSignal Inc. shall not in any case be liable for special, incidental or consequential damages of any kind.

PerkinElmer, Inc. 940 Winter Street Waltham, MA 02451 USA P: (800) 762-4000 or (+1) 203-925-4602 www.perkinelmer.com

