



# BCL-XL/VHL PROTAC BINDING ASSAY KITS

## PROTOCOL

**Part #** 63ADK000CB38PEG & 63ADK000CB38PEH

**Test size:** 500 tests (63ADK000CB38PEG), 10,000 tests (63ADK000CB38PEH) - assay volume: 20  $\mu$ L

**Revision:** 01 (May 2021)

**Store at:** -60°C or below

**For research use only. Not for use in diagnostic procedures.**

### ASSAY PRINCIPLE

The HTRF Bcl-XL/VHL PROTAC Binding Assay is designed to measure the ternary complex formation between Bcl-XL, PROTAC degrader and VHL proteins. Utilizing HTRF (Homogeneous Time-resolved Fluorescence) technology, the assay enables simple and rapid characterization of PROTAC degraders in a high throughput format.

As shown in Figure 1, the interaction between Tag1-Bcl-XL and Tag2-VHL is detected by using anti-Tag1-Europium (HTRF donor) and anti-Tag2-XL665 (HTRF acceptor). When the donor and acceptor antibodies are brought into close proximity due to the Bcl-XL, PROTAC degrader and VHL binding, excitation of the donor antibody triggers fluorescent resonance energy transfer (FRET) towards the acceptor antibody, which in turn emits specifically at 665 nm. This specific signal is directly proportional to the extent of PROTAC degrader bind to both Bcl-XL and VHL protein. Thus, PROTAC degrader forming a ternary complex will cause an increase in HTRF signal.


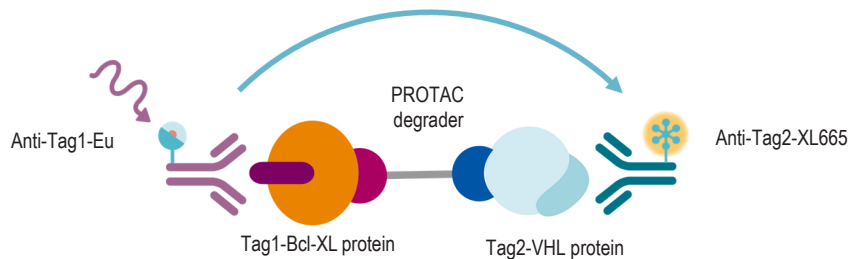


Figure 1: Principle of the HTRF Bcl-XL/VHL PROTAC binding assay.

### PROTOCOL AT A GLANCE

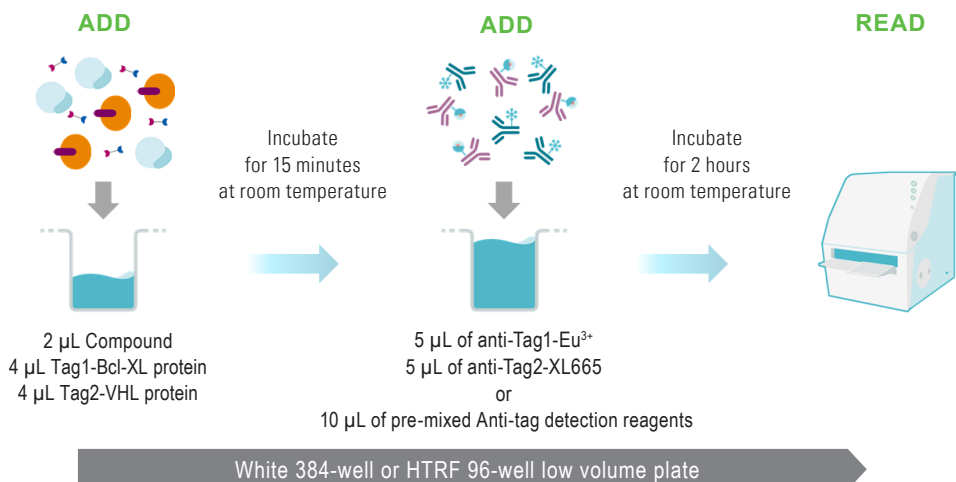

Make sure to use the setup for Eu<sup>3+</sup> Cryptate. For more information about set-up and compatible HTRF® readers, please visit our website at: <http://www.cisbio.com/readers>

**MATERIALS:**

KIT COMPONENTS	500 TESTS CAT # 63ADK000CB38PEG	10,000 TESTS CAT # 63ADK000CB38PEH
Tag1-Bcl-XL* MW: 51.0 kDa	1 vial 25 µL 500X Frozen	1 vial 420 µL 500X Frozen
Tag2-VHL (CUL2/ELOB/ELOC/RBX1) Complex* MW: 153.0 kDa	1 vial 25 µL 500X Frozen	1 vial 420 µL 500X Frozen
PROTAC Standard MW: 1542.4 Da	1 vial 10 µL 3 mM DMSO Solution Frozen	2 vials 10 µL 3 mM DMSO Solution Frozen
Anti-Tag1-Eu <sup>3+</sup>	1 vial 25 µL 100X Frozen	1 vial 0.5 mL 100X Frozen
Anti-Tag2-XL665	1 vial 25 µL 100X Frozen	1 vial 0.5 mL 100X Frozen
Diluent	1 vial 20 mL Cat# 62DLBDDD (200 mL) ready-to-use	1 vial 200 mL Cat# 62DLBDDD (200 mL) ready-to-use
Detection Buffer	1 vial 10 mL Cat# 62DB1FDG (130 mL) ready-to-use	1 vial 130 mL Cat# 62DB1FDG (130 mL) ready-to-use

\* The amounts of Tag1-Bcl-XL and Tag2-VHL provided are sufficient for the validated amounts of tagged proteins suitable for PROTAC ternary complex formation study: optimized concentrations of Bcl-XL and VHL in 20 µL final assay volume.

For reading, an HTRF®-Certified Reader is needed.

For HTRF microplate recommendations, please visit <http://www.cisbio.com/microplate-recommendations>

For a list of HTRF-compatible readers and setup recommendations, please visit <http://www.cisbio.com/readers>

**STORAGE AND STABILITY**

Store the kit at -60°C or below. Under appropriate storage conditions, reagents are stable until the expiry date indicated on the label.



Reagents

Once thawed, tagged Bcl-XL & VHL stock solution may be frozen, and can be thawed only once.

Once thawed (or reconstituted), anti-Tag solutions can be frozen once.

To avoid freeze/thaw cycles, it is recommended to dispense remaining stock solutions into disposable plastic vials for storage at -60°C or below.

Thawed diluent and detection buffer can be stored at 2-8°C on your premises.

**REAGENT PREPARATION****BEFORE YOU BEGIN:**

- It is very important to prepare reagents in the specified buffers. The use of an incorrect diluent may affect reagent stability and assay results.
- Thaw the frozen reagents at room temperature.
- Before use, allow all reagents to warm up to room temperature then homogenize buffer and diluent. It is recommended to filter buffers before use.
- The tagged protein solutions must be prepared in individual vials - DO NOT premix tagged solutions prior to dispensing.
- The anti-Tag solutions must be prepared in individual vials and can be premix prior to dispensing.
- Compounds may be prepared in diluent. We recommend keeping DMSO below 1% during the assay (20 µL final volume).

## TO PREPARE WORKING SOLUTIONS:

Take care to prepare stock and working solutions according to the directions for the kit size you have purchased.

500 TESTS	10,000 TESTS
<b>Tag1-Bcl-XL protein</b> 500X stock solution of optimized final concentration	
Thaw the Tag1-Bcl-XL protein* solution. Dilute 100-fold the 500X Tag1-Bcl-XL protein stock solution with diluent buffer to prepare a 5X working solution. e.g. 5 $\mu$ L of thawed Tag1-Bcl-XL protein stock solution + 495 $\mu$ L of diluent buffer. (20 $\mu$ L final volume).	
<b>Tag2-VHL protein</b> 500X stock solution of optimized final concentration	
Thaw the Tag2-VHL protein* solution. Dilute 100-fold the 500X Tag2-VHL protein stock solution with diluent buffer to prepare a 5X working solution. e.g. 5 $\mu$ L of thawed Tag2-VHL protein stock solution + 495 $\mu$ L of diluent buffer. (20 $\mu$ L final volume).	
<b>Anti-Tag1-Eu<sup>3+</sup></b>	
Thaw the anti-Tag1-Eu <sup>3+</sup> solution. This 100X stock solution can be frozen and stored at -60°C or below. Dilute 100-fold the 100X anti-Tag1-Eu <sup>3+</sup> stock solution with detection buffer.	
e.g. 25 $\mu$ L of thawed anti-Tag1-Eu <sup>3+</sup> stock solution + 2475 $\mu$ L of detection buffer.	e.g. 0.5 mL of thawed anti-Tag1-Eu <sup>3+</sup> stock solution + 49.5 mL of detection buffer.
<b>Anti-Tag2-XL665</b>	
Thaw the anti-Tag2-XL665 solution. This 100X stock solution can be frozen and stored at -60°C or below.  Dilute 100-fold the 100X anti-Tag2-XL665 stock solution with detection buffer. e.g. 25 $\mu$ L of thawed anti-Tag2-XL665 stock solution + 2475 $\mu$ L of detection buffer.	Thaw the anti-Tag2-XL665 solution. This 100X stock solution can be frozen and stored at -60°C or below.  Dilute 100-fold the 100X anti-Tag2-XL665 stock solution with detection buffer. e.g. 0.5 mL of reconstituted anti-Tag2-XL665 stock solution + 49.5 mL of detection buffer.

\*Titration of Tag1-Bcl-XL or Tag2-VHL can be performed if necessary.


## TO PREPARE WORKING PROTAC STANDARD SOLUTIONS:

- Each well requires 2  $\mu$ L of standard.
- In order to counteract any standard sticking, we recommend changing tips between each dilution.

### A recommended standard dilution procedure is listed and illustrated below:


- Dilute the PROTAC standard stock solution 10-fold with diluent buffer to prepare high standard (Std 11):  
Take 4  $\mu$ L of standard stock solution and add it to 36  $\mu$ L of diluent buffer. Mix gently.
- Use the high standard (Std 11) to prepare the standard curve using 3-fold serial dilutions, as follows:
  - Dispense 20  $\mu$ L of diluent buffer into each vial from Std 11 to Std 0.
  - Add 10  $\mu$ L of standard to 20  $\mu$ L of diluent buffer, mix gently, and repeat the serial dilution to make the other standard solutions: Std10, Std9, Std8, Std7, Std6, Std5, Std4, Std3, Std2, Std1.

This will create 11 standards for the analyte. Std 0 (Negative control) is diluent buffer.

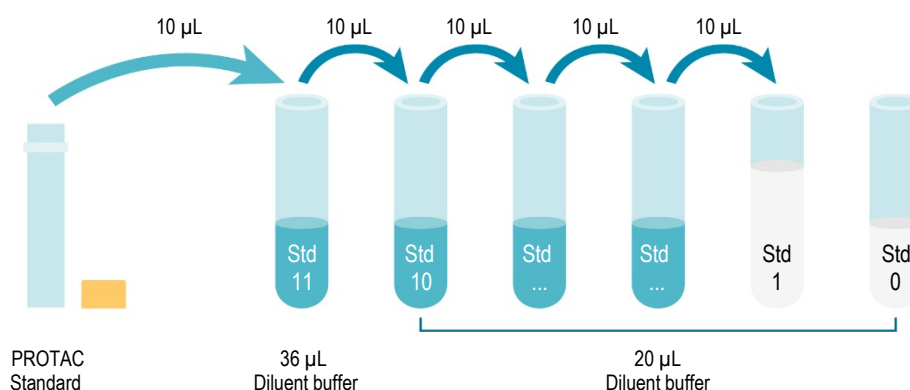

STANDARD	SERIAL DILUTIONS	WORKING SOLUTIONS	FINAL CONCENTRATIONS
Standard stock solution	Thawed stock solution	3 000 µM	
Standard 11	4 µL standard stock solution + 36 µL Diluent buffer	300 µM	30 µM
Standard 10	10 µL Standard 11 + 20 µL Diluent buffer	100 µM	10 µM
Standard 9	10 µL Standard 10 + 20 µL Diluent buffer	33 µM	3.3 µM
Standard 8	10 µL Standard 9 + 20 µL Diluent buffer	11 µM	1.1 µM
Standard 7	10 µL Standard 8 + 20 µL Diluent buffer	3.7 µM	0.37 µM
Standard 6	10 µL Standard 7 + 20 µL Diluent buffer	1.2 µM	0.12 µM
Standard 5	10 µL Standard 6 + 20 µL Diluent buffer	0.41 µM	0.041 µM
Standard 4	10 µL Standard 5 + 20 µL Diluent buffer	0.14 µM	0.014 µM
Standard 3	10 µL Standard 4 + 20 µL Diluent buffer	0.046 µM	0.0046 µM
Standard 2	10 µL Standard 3 + 20 µL Diluent buffer	0.015 µM	0.0015 µM
Standard 1	10 µL Standard 2 + 20 µL Diluent buffer	0.005 µM	0.0005 µM
Standard 0	20 µL Diluent buffer	0 µM	0 µM

## ASSAY PROTOCOL

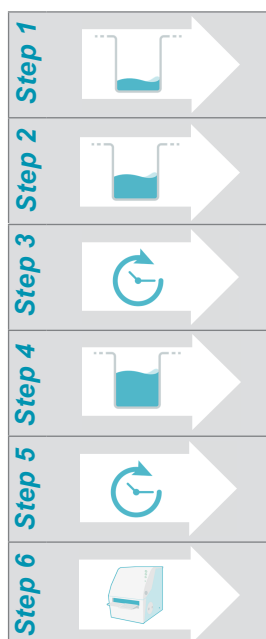

Cryptate control	Standard (Std 0 - Std 11)	Compound
Dispense 10 µL of diluent buffer into each cryptate control well.	Dispense 2 µL of each PROTAC standard (Std 0 - Std 11) into each standard well.	Dispense 2 µL of compound into each compound well.
	Add 4 µL of Tag1-Bcl-XL protein and 4 µL of Tag2-VHL protein to all wells.	
Incubate for 15 minutes at room temperature.		
Dispense 5 µL of anti-Tag1-Eu3+ and 5 µL of detection buffer.	Dispense 10 µL of pre-mixed anti-Tag1-Eu3+ and anti-Tag2-XL665.	
Seal the plate and incubate for 2 hours at room temperature.		
Remove the plate sealer and read on an HTRF® compatible reader.		

## EXAMPLE OF PLATE MAP

	1	2	3	4	5	6
<b>A</b>	<b>Buffer control:</b> 10 µL diluent 10 µL detection buffer	Repeat Well A1	Repeat Well A1	<b>Compound...:</b> 2 µL compound... 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well A4	Repeat Well A4
<b>B</b>	<b>Cryptate control:</b> 10 µL diluent 5 µL detection buffer 5 µL anti-Tag1-Eu	Repeat Well B1	Repeat Well B1	<b>Compound...:</b> 2 µL compound... 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well B4	Repeat Well B4
<b>C</b>	<b>Negative control:</b> 2 µL diluent 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well C1	Repeat Well C1	<b>Compound...:</b> 2 µL compound... 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well C4	Repeat Well C4
<b>D</b>	<b>Positive control:</b> 2 µL PROTAC standard 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well D1	Repeat Well D1	<b>Compound...:</b> 2 µL compound... 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well D4	Repeat Well D4
<b>E</b>	<b>Compound 1:</b> 2 µL compound 1 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well E1	Repeat Well E1	<b>Compound...:</b>	Repeat Well E4	Repeat Well E4
<b>F</b>	<b>Compound 2:</b> 2 µL compound 2 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well F1	Repeat Well F1	<b>Compound...:</b>	Repeat Well F4	Repeat Well F4
<b>G</b>	<b>Compound...:</b> 2 µL compound... 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well G1	Repeat Well G1	<b>Compound...:</b>	Repeat Well G4	Repeat Well G4
<b>H</b>	<b>Compound...:</b> 2 µL compound... 4 µL Tag1-Bcl-XL 4 µL Tag2-VHL 10 µL pre-mix anti-Tag reagents	Repeat Well H1	Repeat Well H1			

## DATA REDUCTION & INTERPRETATION

1. Calculate the ratio of the acceptor and donor emission signals for each individual well.

$$\text{Ratio} = \frac{\text{Signal 665 nm}}{\text{Signal 620 nm}} \times 10^4$$

2. Calculate the % CVs. The mean and standard deviation can then be worked out from ratio replicates.

$$\text{CV (\%)} = \frac{\text{Standard deviation}}{\text{Mean Ratio}} \times 100$$

For more information about data reduction, please visit <http://www.cisbio.com/data-reduction>

The data should be fitted with Bell-shaped equation in GraphPad Prism software.

## RESULTS

The data shown below must not be substituted for the data obtained in the laboratory, and should be considered only as an example.


The formation of ternary complex were tested at optimized concentrations of VHL and Bcl-XL.

Readouts on **PerkinElmer® EnVision** with a flash lamp.

Note that results may vary from one HTRF® compatible reader to another.

Compound	Vender	Cat#	Description
DT2216	MCE	HY-130604	A potent PROTAC degrader which causes effective degradation of Bcl-XL protein by recruiting E3 ubiquitin ligase VHL.
XZ739	MCE	HY-133557	A CRBN-dependent PROTAC Bcl-XL degrader which can induce cell death through caspase-mediated apoptosis.
MZ-1	MCE	HY-107425	A long-lasting and selective removal degrader based PROTAC between BRD4 and VHL.
Navitoclax	MCE	HY-10087	An orally active Bcl-2 family protein inhibitor and it can be used in the synthesis of PROTAC DT2216.
VH032	MCE	HY-120217	A ligand used in the recruitment of the VHL protein, and it is used as a precursor to synthesise MZ-1.
ABT-737	Selleck	S1002	A BH3 mimetic inhibitor of Bcl-XL, Bcl-2 which induces mitochondrial pathway apoptosis and mitophagy.

**Bcl-XL/VHL PROTAC binding assay  
Ternary complex formation**

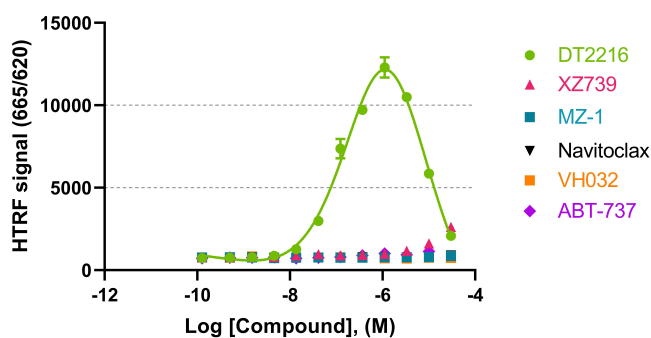

The concentration of DT2216 at peak, 1111 nM

This product contains material of biologic origin. Use for research purposes only. Do not use in humans or for diagnostic purposes. The purchaser assumes all risk and responsibility concerning reception, handling and storage.  
Copyright 2020 Cisbio, France. All rights reserved. HTRF®, Tag-lite®, and EPIgeneous™ are trademarks or registered trademarks of Cisbio. All other trademarks are the property of their respective owners.

### FOR MORE INFORMATION

Europe and other countries +33(0)466-796-705 U.S. and Canada 1-888-963-4567 China +86-21-5018-9880  
Japan +81-(0)43-306-8712 Visit [www.cisbio.com](http://www.cisbio.com) to find a list of our regional distributors



cisbio